



Laundering and Care

1. Remove all panels and/ or any metal components prior to cleaning.
2. This brace can be hand washed in cold or lukewarm water with mild soap or detergent and air dried
3. Do not use any substance containing Chlorine

Warning

1. Carefully read this application instruction and warning prior to fitting braces, failure to properly position the brace and fasten each strap will compromise performance and support.
2. This brace will NOT prevent or reduce all injuries. Proper rehabilitation and activity modification are essential while wearing the brace.
3. Federal Law restricts the sale of this Device to anyone other than a Licensed Health Care Provider.

Caution

1. Single patient use only
2. Do not over-tighten closures
3. If irritation, pain or discomfort occurs while wearing this brace, discontinue use and immediately consult your medical professional.

EUROPEAN AUTHORIZED REPRESENTATIVE



Wellkang Ltd
Suite B, 29 Harley Street,
LONDON, W1G 9QR, U.K.
www.CE-Marking.EU



Council Directive
93/42/EEC of
14 June 1993
concerning Medical Device

MANUFACTURED BY

Dicarre LLC

info@dicarre.com

Toll Free: 1-844-DICARRE

125 Half Mile Road, Suite 200
Red Bank, NJ 07701


www.dicarre.com

DICARRE

Dicarre Noble™ Sling
ER 90°

DE21

User Guide
Application Instruction

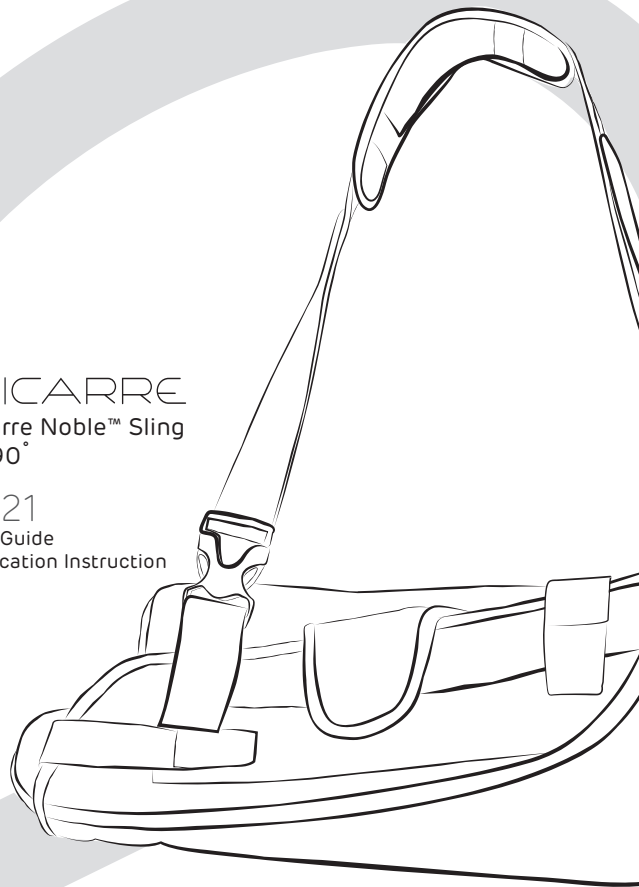

1. The brace is pre-assembled for a right arm. If the left arm is applied, detach the sling from the pillow, flip, and reattach.

2. While supporting the affected arm, slide the forearm into sling. Wrap the adjustable shoulder strap around the neck and shoulders and attach the strap end to the sling using the alligator strap tab.(Fig. 1)

3. Adjust the shoulder strap to the required length and the shoulder pad to the desired position.(Fig. 2)

4. Adjust the sling length by folding back the sling at the wrist. Note: For a small size detach and move the shoulder strap to the wrist.(Fig. 3)

5. Attach the closure strap across the open top of the sling. Position the strap so that it holds the arm securely in the sling. Attach the thumb strap to the open end of the sling between the thumb and fingers.(Fig. 4)

6. If a neutral pillow or 15°/ER90° abduction pillow is included, place the pillow at the waistline. Attach the sling to the pillow, lining up hook material on the pillow with the loop on sling. Adjust the waist strap to fit.(Fig. 5)

